


Sample Name: MEOH

```
=====
Acq. Operator   :                               Seq. Line :    1
Acq. Instrument : Instrument 2                   Location  : Vial 51
Injection Date  : 6/24/2026 12:28:37 PM          Inj       :    1
                                                Inj Volume : 0 µl
Acq. Method     : C:\CHEM32\2\DATA\06242026\JV 06242026 C 2026-06-24 12-18-50\HS FID ROH
                                                06232026.M
Last changed    : 6/24/2026 8:43:02 AM
Analysis Method : C:\CHEM32\2\METHODS\DEF_GC.M
Last changed    : 6/25/2026 9:13:32 AM
                  (modified after loading)
=====
```

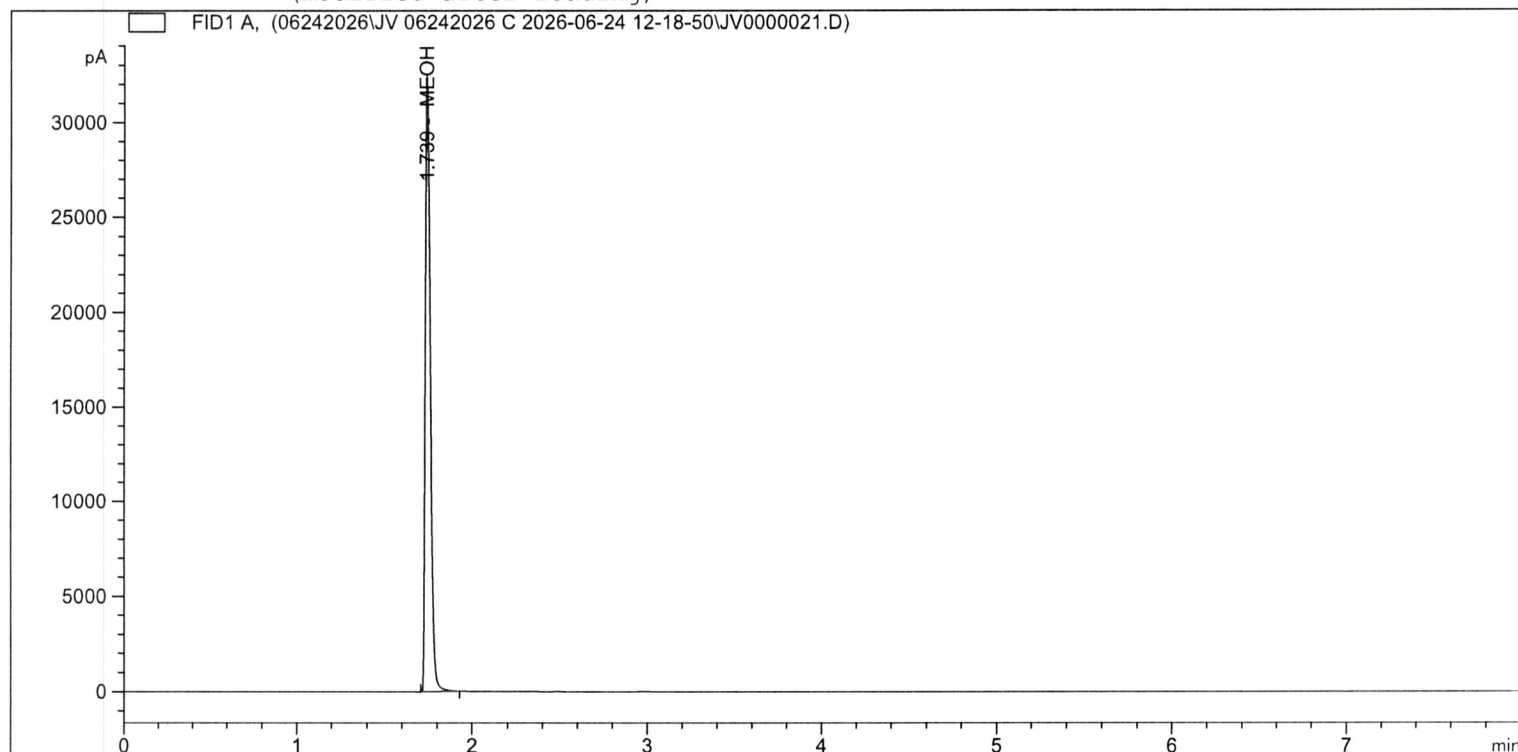

=====
Area Percent Report
=====

```
Sorted By      :      Signal
Calib. Data Modified : 6/25/2026 9:12:23 AM
Multiplier:      :      1.0000
Dilution:        :      1.0000
Use Multiplier & Dilution Factor with ISTDs
```

Signal 1: FID1 A,

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
1	1.739	BB S	0.0302	6.38319e4	1.000e2	MEOH
2	3.089		0.0000	0.00000	0.00000	ACN

Totals : 6.38319e4

2 Warnings or Errors :


Warning : Calibrated compound(s) not found

Warning : Invalid calibration curve, (MEOH)

=====
*** End of Report ***

Sample Name: ACN

```
=====
Acq. Operator   :                               Seq. Line :    2
Acq. Instrument : Instrument 2                  Location  : Vial 52
Injection Date  : 6/24/2026 12:52:21 PM        Inj       :    1
                                                Inj Volume: 0 µl
Acq. Method     : C:\CHEM32\2\DATA\06242026\JV 06242026 C 2026-06-24 12-18-50\HS FID ROH
                                                06232026.M
Last changed    : 6/24/2026 8:43:02 AM
Analysis Method : C:\CHEM32\2\METHODS\DEF_GC.M
Last changed    : 6/25/2026 9:13:32 AM
                (modified after loading)
=====
```

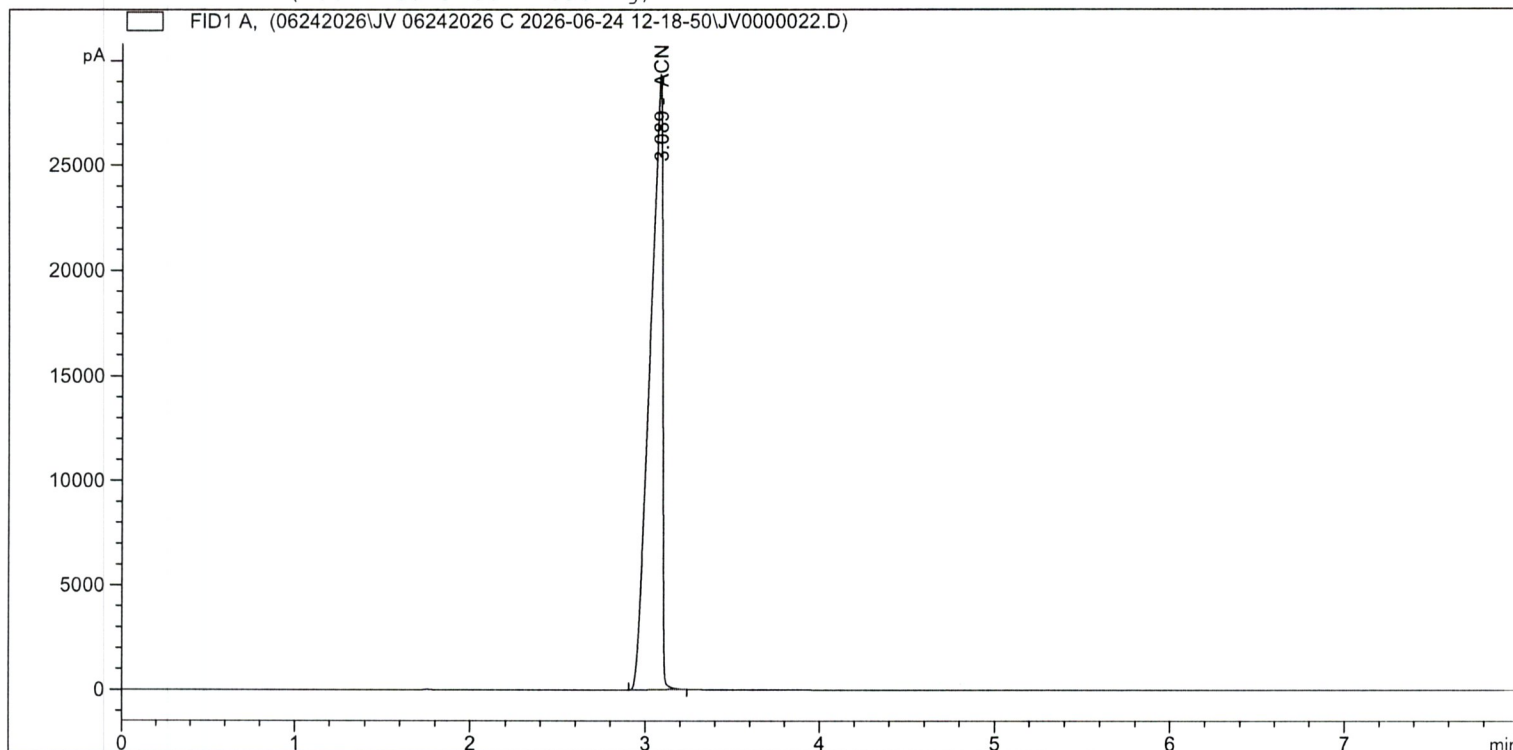

=====
Area Percent Report
=====

```
Sorted By      :      Signal
Calib. Data Modified : 6/25/2026 9:12:23 AM
Multiplier:      :      1.0000
Dilution:        :      1.0000
Use Multiplier & Dilution Factor with ISTDs
```

Signal 1: FID1 A,

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
1	1.739		0.0000	0.00000	0.00000	MEOH
2	3.089	BB S	0.0624	1.45384e5	1.000e2	ACN

Totals : 1.45384e5


2 Warnings or Errors :

Warning : Calibrated compound(s) not found

Warning : Invalid calibration curve, (ACN)

=====
*** End of Report ***

```
=====
Acq. Operator   :                               Seq. Line :    3
Acq. Instrument : Instrument 2                   Location  : Vial 53
Injection Date  : 6/24/2026 1:16:03 PM           Inj       :    1
                                                Inj Volume : 0 µl
Acq. Method     : C:\CHEM32\2\DATA\06242026\JV 06242026 C 2026-06-24 12-18-50\HS FID ROH
                                                06232026.M
Last changed    : 6/24/2026 8:43:02 AM
Analysis Method : C:\CHEM32\2\METHODS\DEF_GC.M
Last changed    : 6/25/2026 9:13:32 AM
                (modified after loading)
=====
```

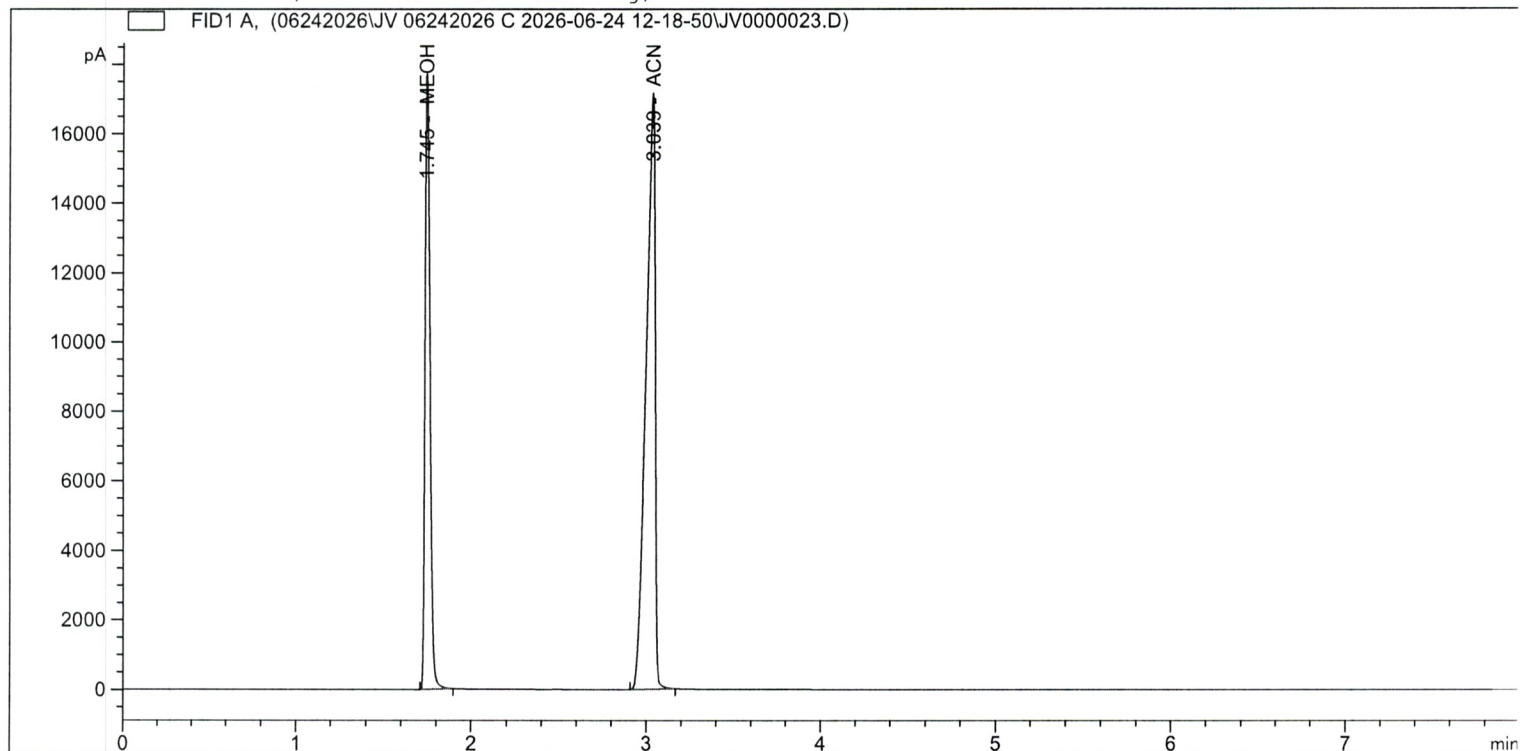

```
=====
                        Area Percent Report
=====
```

```
Sorted By      :      Signal
Calib. Data Modified :      6/25/2026 9:12:23 AM
Multiplier:      :      1.0000
Dilution:      :      1.0000
Use Multiplier & Dilution Factor with ISTDs
```

Signal 1: FID1 A,

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
1	1.745	BB S	0.0300	3.44447e4	35.71166	MEOH
2	3.039	BB S	0.0475	6.20075e4	64.28834	ACN

Totals : 9.64521e4

2 Warnings or Errors :

Sample Name: SPL

Warning : Invalid calibration curve, (MEOH)


Warning : Invalid calibration curve, (ACN)

=====
*** End of Report ***

Sample Name: SPL

=====

Acq. Operator	:		Seq. Line	:	4
Acq. Instrument	:	Instrument 2	Location	:	Vial 54
Injection Date	:	6/24/2026 1:39:44 PM	Inj	:	1
			Inj Volume	:	0 µl
Acq. Method	:	C:\CHEM32\2\DATA\06242026\JV 06242026 C 2026-06-24 12-18-50\HS FID ROH 06232026.M			
Last changed	:	6/24/2026 8:43:02 AM			
Analysis Method	:	C:\CHEM32\2\METHODS\DEF_GC.M			
Last changed	:	6/25/2026 9:13:32 AM			
		(modified after loading)			

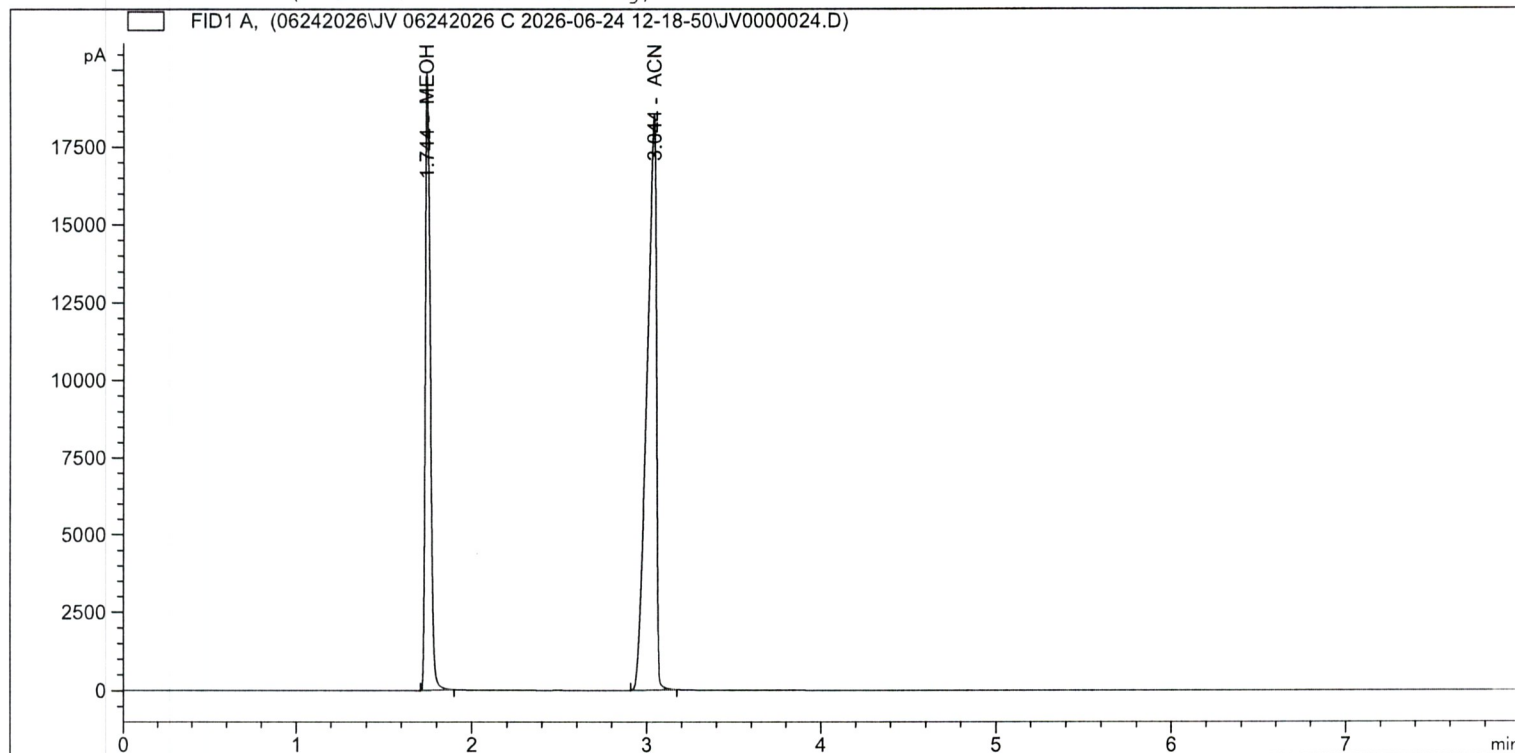

=====
Area Percent Report
=====

Sorted By : Signal
Calib. Data Modified : 6/25/2026 9:12:23 AM
Multiplier: : 1.0000
Dilution: : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: FID1 A,

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
1	1.744	BB S	0.0302	3.86126e4	35.78116	MEOH
2	3.044	BB S	0.0485	6.93005e4	64.21884	ACN

Totals : 1.07913e5

2 Warnings or Errors :

Sample Name: SPL


Warning : Invalid calibration curve, (MEOH)

Warning : Invalid calibration curve, (ACN)

=====
*** End of Report ***

Sample Name: SPL

```
=====
Acq. Operator   :                               Seq. Line :    5
Acq. Instrument : Instrument 2                  Location  : Vial 55
Injection Date  : 6/24/2026 2:03:25 PM          Inj       :    1
                                                Inj Volume: 0 µl
Acq. Method     : C:\CHEM32\2\DATA\06242026\JV 06242026 C 2026-06-24 12-18-50\HS FID ROH
                                                06232026.M
Last changed    : 6/24/2026 8:43:02 AM
Analysis Method : C:\CHEM32\2\METHODS\DEF_GC.M
Last changed    : 6/25/2026 9:13:32 AM
                (modified after loading)
=====
```

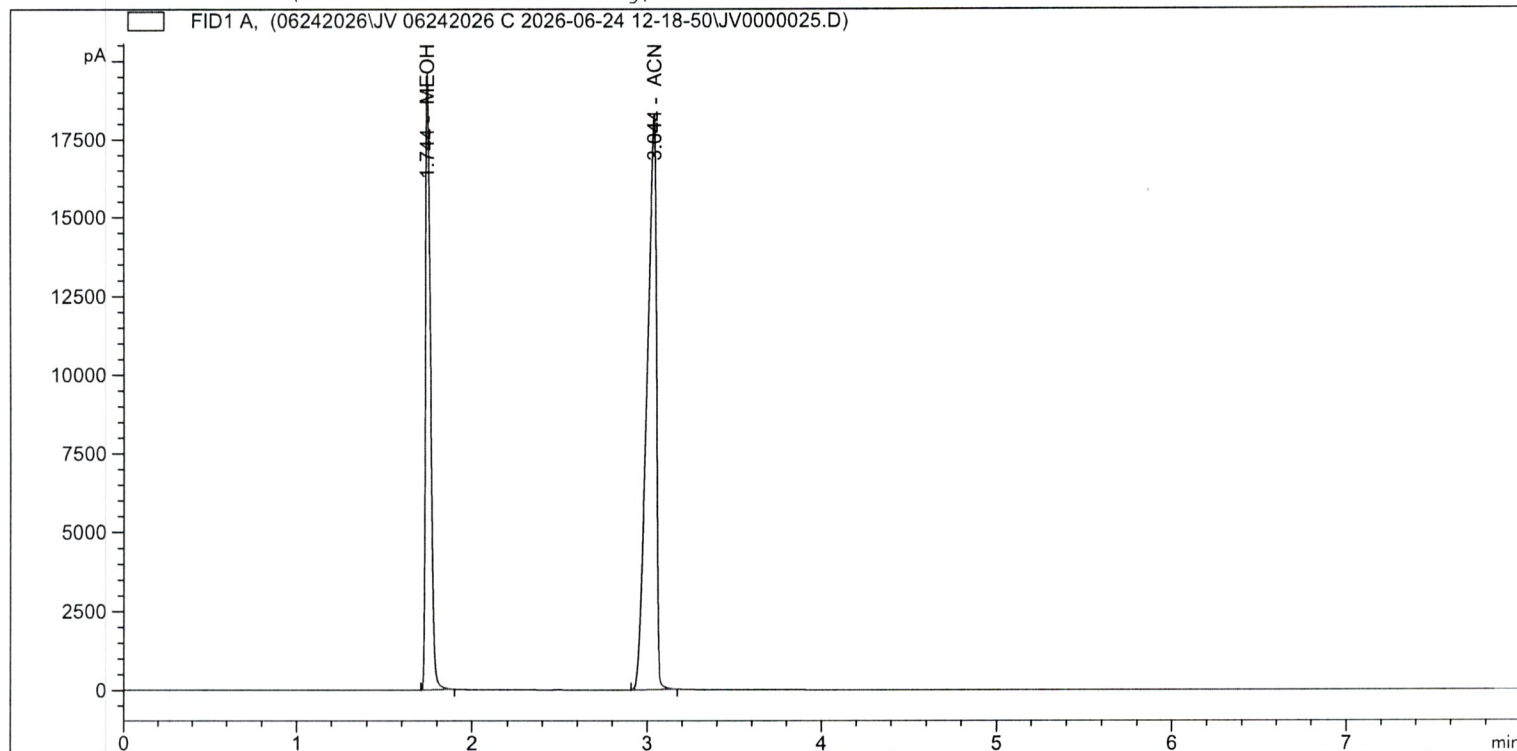

=====
Area Percent Report
=====

```
Sorted By      :      Signal
Calib. Data Modified : 6/25/2026 9:12:23 AM
Multiplier:      :      1.0000
Dilution:        :      1.0000
Use Multiplier & Dilution Factor with ISTDs
```

Signal 1: FID1 A,

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
1	1.744	BB S	0.0302	3.80672e4	35.90946	MEOH
2	3.044	BB S	0.0486	6.79416e4	64.09054	ACN

Totals : 1.06009e5

2 Warnings or Errors :


Warning : Invalid calibration curve, (MEOH)

Warning : Invalid calibration curve, (ACN)

=====
*** End of Report ***

=====

Acq. Operator	:		Seq. Line	:	6
Acq. Instrument	:	Instrument 2	Location	:	Vial 56
Injection Date	:	6/24/2026 2:27:03 PM	Inj	:	1
			Inj Volume	:	0 µl
Acq. Method	:	C:\CHEM32\2\DATA\06242026\JV 06242026 C 2026-06-24 12-18-50\HS FID ROH 06232026.M			
Last changed	:	6/24/2026 8:43:02 AM			
Analysis Method	:	C:\CHEM32\2\METHODS\DEF_GC.M			
Last changed	:	6/25/2026 9:13:32 AM			
		(modified after loading)			

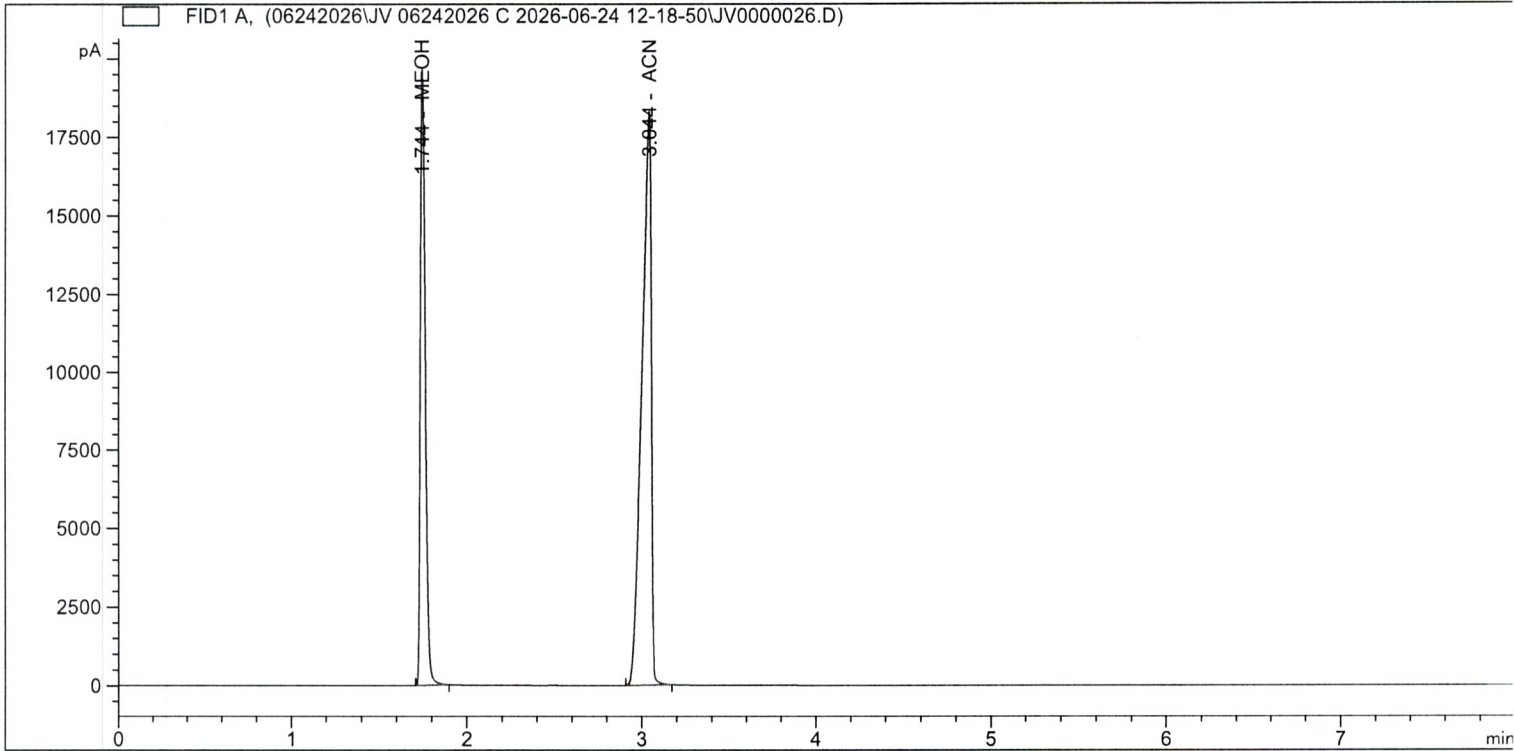

=====
Area Percent Report
=====

Sorted By : Signal
Calib. Data Modified : 6/25/2026 9:12:23 AM
Multiplier: : 1.0000
Dilution: : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: FID1 A,

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
1	1.744	BB S	0.0299	3.82104e4	35.98093	MEOH
2	3.044	BB S	0.0495	6.79859e4	64.01907	ACN

Totals : 1.06196e5


2 Warnings or Errors :

Warning : Invalid calibration curve, (MEOH)
Warning : Invalid calibration curve, (ACN)

=====
*** End of Report ***

=====

Acq. Operator	:		Seq. Line	:	7
Acq. Instrument	:	Instrument 2	Location	:	Vial 57
Injection Date	:	6/24/2026 2:50:44 PM	Inj	:	1
			Inj Volume	:	0 µl
Acq. Method	:	C:\CHEM32\2\DATA\06242026\JV 06242026 C 2026-06-24 12-18-50\HS FID ROH 06232026.M			
Last changed	:	6/24/2026 8:43:02 AM			
Analysis Method	:	C:\CHEM32\2\METHODS\DEF_GC.M			
Last changed	:	6/25/2026 9:13:32 AM			
		(modified after loading)			

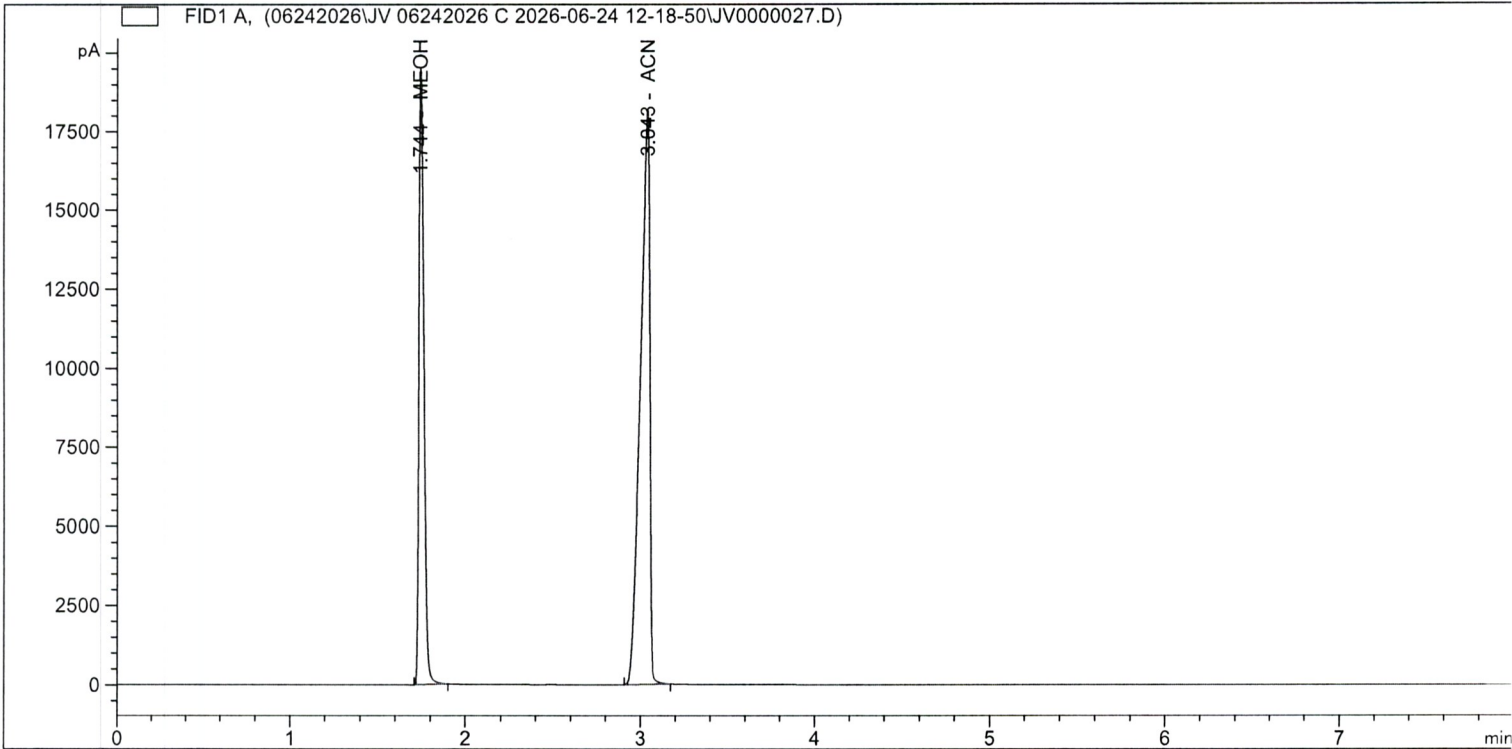

=====
Area Percent Report
=====

Sorted By : Signal
Calib. Data Modified : 6/25/2026 9:12:23 AM
Multiplier: : 1.0000
Dilution: : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: FID1 A,

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
1	1.744	BB S	0.0303	3.78497e4	35.96436	MEOH
2	3.043	BB S	0.0488	6.73926e4	64.03564	ACN

Totals : 1.05242e5

2 Warnings or Errors :

Sample Name: SPL


Warning : Invalid calibration curve, (MEOH)

Warning : Invalid calibration curve, (ACN)

=====
*** End of Report ***

Sample Name: SPL

```
=====
Acq. Operator   :                               Seq. Line :    8
Acq. Instrument : Instrument 2                   Location  : Vial 58
Injection Date  : 6/24/2026 3:14:22 PM           Inj       :    1
                                                Inj Volume : 0 µl
Acq. Method     : C:\CHEM32\2\DATA\06242026\JV 06242026 C 2026-06-24 12-18-50\HS FID ROH
                                                06232026.M
Last changed    : 6/24/2026 8:43:02 AM
Analysis Method : C:\CHEM32\2\METHODS\DEF_GC.M
Last changed    : 6/25/2026 9:13:32 AM
                  (modified after loading)
=====
```

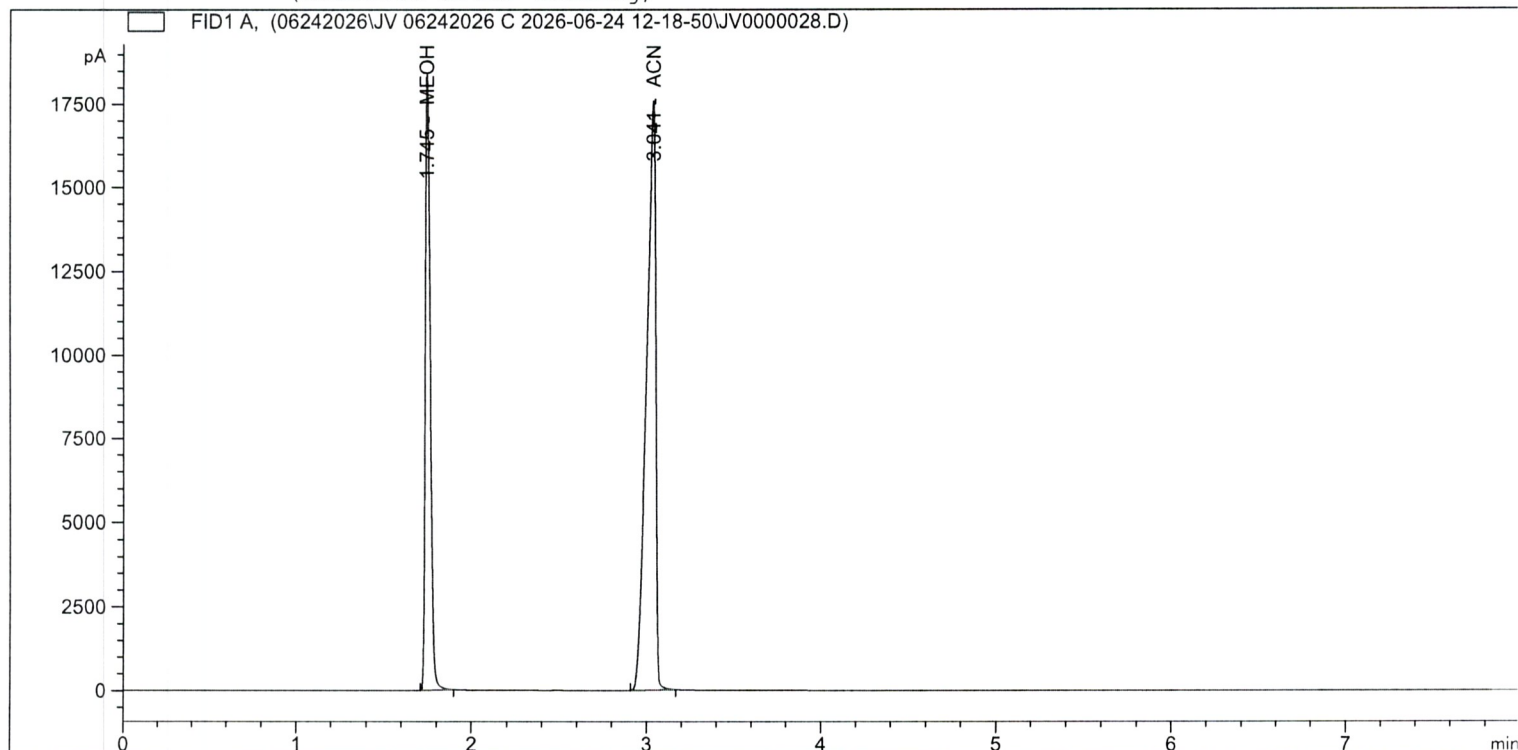

=====
Area Percent Report
=====

Sorted By : Signal
Calib. Data Modified : 6/25/2026 9:12:23 AM
Multiplier: : 1.0000
Dilution: : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: FID1 A,

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
1	1.745	BB S	0.0302	3.57730e4	35.81073	MEOH
2	3.041	BB S	0.0486	6.41216e4	64.18927	ACN

Totals : 9.98945e4

2 Warnings or Errors :

Sample Name: SPL

Warning : Invalid calibration curve, (MEOH)

Warning : Invalid calibration curve, (ACN)

=====
*** End of Report ***